

For professional use only.  
For in vitro diagnostic use only.

**[INTENDED USE]**

The COVID-19 Antigen Rapid Test Cassette is a lateral flow immunoassay intended for the qualitative detection SARS-CoV-2 nucleocapsid antigens in nasopharyngeal swab and oropharyngeal swab from individuals who are suspected of COVID-19 by their healthcare provider.

Results are for the identification of SARS-CoV-2 nucleocapsid antigen. Antigen is generally detectable in nasopharyngeal swab and oropharyngeal swab during the acute phase of infection. Positive results indicate the presence of viral antigens, but clinical correlation with patient history and other diagnostic information is necessary to determine infection status. Positive results do not rule out bacterial infection or co-infection with other viruses. The agent detected may not be the definite cause of disease.

Negative results do not rule out SARS-CoV-2 infection and should not be used as the sole basis for treatment or patient management decisions, including infection control decisions. Negative results should be considered in the context of a patient's recent exposures, history and the presence of clinical signs and symptoms consistent with COVID-19, and confirmed with a molecular assay, if necessary for patient management.

The COVID-19 Antigen Rapid Test Cassette is intended for use by trained clinical laboratory personnel specifically instructed and trained in vitro diagnostic procedures.

**[SUMMARY]**

The novel coronaviruses (SARS-CoV-2) belong to the β genus. COVID-19 is an acute respiratory infectious disease. People are generally susceptible. Currently, the patients infected by the novel coronavirus are the main source of infection; asymptomatic infected people can also be an infectious source. Based on the current epidemiological investigation, the incubation period is 1 to 14 days, mostly 3 to 7 days. The main manifestations include fever, fatigue and dry cough. Nasal congestion, runny nose, sore throat, myalgia and diarrhea are found in a few cases.

**[PRINCIPLE]**

The COVID-19 Antigen Rapid Test is a lateral flow immunoassay based on the principle of the double-antibody sandwich technique. SARS-CoV-2 nucleocapsid protein monoclonal antibody conjugated with color microparticles is used as detector and sprayed on conjugation pad. During the test, SARS-CoV-2 antigen in the specimen interacts with SARS-CoV-2 antibody conjugated with color microparticles making antigen-antibody labeled complex. This complex migrates on the membrane via capillary action until the test line, where it will be captured by the pre-coated SARS-CoV-2 nucleocapsid protein monoclonal antibody. A colored test line (T) would be visible in the result window if SARS-CoV-2 antigens are present in the specimen. Absence of the T line suggests a negative result. The control line (C) is used for procedural control, and should always appear if the test procedure is performed properly.

**[WARNINGS AND PRECAUTIONS]**

- For in vitro diagnostic use only.
- For healthcare professionals and professionals at point of care sites.
- Do not use this product as the sole basis to diagnose or exclude SARS-CoV-2 infection or to inform infection status of COVID-19.
- Do not use after the expiration date.

- Please read all the information in this leaflet before performing the test.
- The test cassette should remain in the sealed pouch until use.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used test cassette should be discarded according to federal, state and local regulations.

**[COMPOSITION]**

**Materials Provided**

- 25 Test Cassettes: each cassette with desiccant in individual foil pouch
- 25 Extraction Reagent: ampoule containing 0.3 mL of extraction reagent
- 25 Sterilized Swabs: single use swab for specimen collection
- 25 Extraction Tubes
- 25 Dropper Tips
- 1 Work Station
- 1 Package Insert

**Materials Required but not Provided**

- Timer

**[STORAGE AND STABILITY]**

- Store as packaged in the sealed pouch at temperature (4-30°C or 40-86°F). The kit is stable within the expiration date printed on the labeling.
- Once open the pouch, the test should be used within one hour. Prolonged exposure to hot and humid environment will cause product deterioration.
- The LOT and the expiration date were printed on the labeling.


**[SPECIMEN]**

Specimens obtained early during symptom onset will contain the highest viral titers; specimens obtained after five days of symptoms are more likely to produce negative results when compared to an RT-PCR assay. Inadequate specimen collection, improper specimen handling and/or transport may yield false results; therefore, training in specimen collection is highly recommended due to the importance of specimen quality to obtain accurate test results.

Acceptable specimen type for testing is a direct swab specimen or a swab in viral transport media (VTM) without denaturing agents.

Prepare the extraction tube according to the Test Procedure and use the sterile swab provided in the kit for specimen collection.


**Nasopharyngeal Swab Specimen Collection**

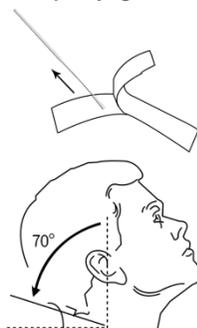


1. Remove the swab from the package.

2. Tilt patient's head back about 70°.

3. Insert the swab through the nostril parallel to the palate (not upwards) until resistance is encountered or the distance is equivalent to that from the ear to the nostril of the patient, indicating contact with the nasopharynx. (Swab should



reach depth equal to distance from nostrils to outer opening of the ear.) Gently rub and roll the swab. Leave swab in place for several seconds to absorb secretions.



4. Slowly remove swab while rotating it.

Specimens can be collected from both sides using the same swab, but it is not necessary to collect specimens from both sides if the minitip is saturated with fluid from the first collection. If a deviated septum or blockage creates difficulty in obtaining the specimen from one nostril, use the same swab to obtain the specimen from the other nostril.

**Oropharyngeal Swab Specimen Collection**



Insert swab into the posterior pharynx and tonsillar areas. Rub swab over both tonsillar pillars and posterior oropharynx and avoid touching the tongue, teeth, and gums.


**Specimen Transport and Storage**

Do not return the swab to the original swab packaging. Freshly collected specimens should be processed as soon as possible, but no later than one hour after specimen collection. Specimen collected may be stored at 2-8°C for no more than 24 hours; Store at -70°C for a long time, but avoid repeated freeze-thaw cycles.

**[TEST PROCEDURE]**


**Note:** Allow the test devices, reagents and specimens to equilibrate to room temperature (15-30°C or 59-86°F) prior to testing.

- Put an extraction tube on the work station.
- Unscrew the lid of an extraction reagent. Add all of the extraction reagent into an extraction tube.
- Sampling refer to section 'Specimen Collection'.

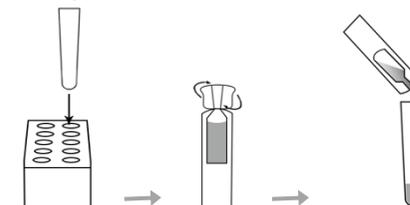


**Direct Swab Test Procedure**

1. Insert the swab specimen into the extraction tube which contains extraction reagent. Roll the swab at least 5 times while pressing the head against the bottom and side of the extraction tube. **Leave the swab in the extraction tube for one minute.**
2. Remove the swab while squeezing the sides of the tube to extract the liquid from the swab. The extracted solution will be used as test sample.
3. Cover the extraction tube with a dropper tip tightly.

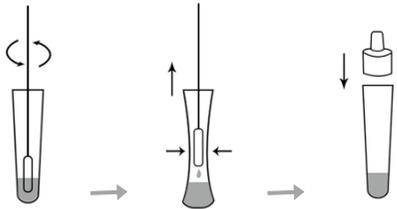


- Remove the test cassette from the sealed pouch.
- Reverse the specimen extraction tube, holding the tube upright, transfer 3 drops (approximately 100µL) slowly to the specimen well (S) of the test cassette, then start the timer.
- Wait for colored lines to appear. Interpret the test results **at 15 minutes**. Do not read results after 20 minutes.

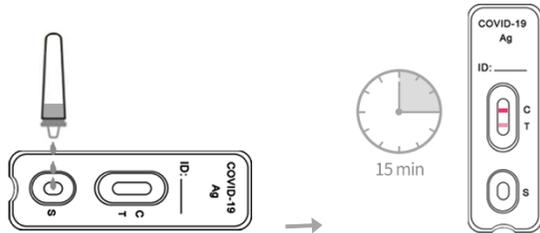

#### Swab in Viral Transport Media (VTM) Test Procedure

- Insert the swab specimen into the transport tube containing a maximum of 3 mL VTM without denaturing agents.
- Mix the specimen stored in VTM by vortexing.
- Transfer 300µL of the VTM solution containing specimen into the extraction tube which contains extraction reagent with a calibrated micropipette. Homogenise mixture by pipetting up and down.
- Cover the extraction tube with a dropper tip tightly, **and let the extracted solution stand for one minute**.

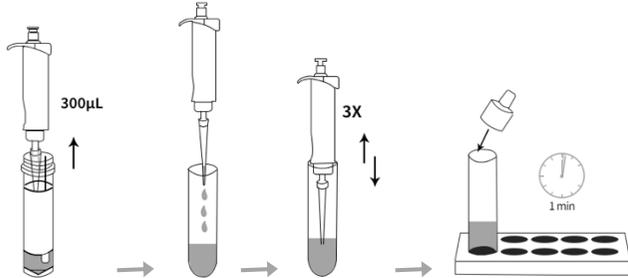

- Follow Steps 4 – 6 of the **Direct Swab Test Procedure** above.

#### [INTERPRETATION OF RESULTS]

<b>Positive</b>		<b>Two lines appear.</b> One colored line appears at the control region (C), and another colored line appears at the test region (T), regardless of the intensity of the test line.
<b>Negative</b>		One colored line appears at the control region (C), and no line appears at the test region (T).

**Invalid**

**Control line fails to appear.** Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test using a new test cassette. If the problem persists, discontinue using the lot immediately and contact your local distributor.

#### [QUALITY CONTROL]

A procedural control is included in the test. A colored line appearing in the control region (C) is considered an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique.

Control standards are not supplied with this kit. However, it is recommended that positive and negative controls be tested as good laboratory practice to confirm the test procedure and to verify proper test performance.

#### [LIMITATIONS]

- The product is limited to provide a qualitative detection. The intensity of the test line does not necessarily correlate to the concentration of the antigen of the specimens.
- Negative results do not preclude SARS-CoV-2 infection and should not be used as the sole basis for patient management decisions.
- A physician must interpret the results in conjunction with the patient's history, physical findings, and other diagnostic procedures.
- A negative result can occur if the quantity of SARS-CoV-2 antigens present in the specimen is below the detection threshold of the assay, or the virus has undergone minor amino acid mutation(s) in the target epitope region recognized by the monoclonal antibodies utilized in the test.

#### [PERFORMANCE CHARACTERISTICS]

##### Clinical Performance

To estimate the clinical performance between the COVID-19 Antigen Rapid Test Cassette and the RT-PCR comparator, 285 nasopharyngeal swabs were collected from individual symptomatic patients (within 7 days of onset) who were suspected of COVID-19.

Summary data of COVID-19 Antigen Rapid Test as below:

COVID-19 Antigen	RT-PCR		Total
	Positive	Negative	
<b>CLUNGENE®</b> Positive	64	0	64
Negative	6*	215	221
<b>Total</b>	70	215	285

Sensitivity (PPA)= 91.4% (64/70), (95%CI: 82.5%~96.0%)

Specificity (NPA)= 100% (215/215), (95%CI: 98.2%~100%)

\*The 6 discordant specimens had Ct values of 34, 36, 35.5, 34, 35, 33.

The PPA is 98.5% (64/65) (95%CI: 91.8%~99.7%) with specimens of a Ct count ≤33.

##### Limit of Detection (Analytical Sensitivity)

The study used cultured SARS-CoV-2 virus, which is β-propiolactone and heat inactivated and spiked into nasopharyngeal swab specimen. The Limit of Detection (LoD) is  $5 \times 10^{2.67}$  TCID<sub>50</sub>/mL.

##### Cross Reactivity (Analytical Specificity)

Cross reactivity was evaluated by testing 32 commensal and pathogenic microorganisms that may be present in the nasal cavity.

No cross-reactivity was observed with recombinant MERS-CoV NP protein when tested at the concentration of 50 µg/mL.

No cross-reactivity was observed with the following viruses when tested at the concentration of  $1.0 \times 10^6$  PFU/mL: Influenza A (H1N1), Influenza A (H1N1pdm09), Influenza A (H3N2), Influenza B (Yamagata), Influenza B (Victoria), Adenovirus (type 1, 2, 3, 5, 7, 55), Human metapneumovirus, Parainfluenza virus (type 1, 2, 3, 4), Respiratory syncytial virus, Enterovirus, Rhinovirus, Human coronavirus 229E, Human coronavirus OC43, Human coronavirus NL63, Human coronavirus HKU1.

No cross-reactivity was observed with the following bacteria when tested at the concentration of  $1.0 \times 10^7$  CFU/mL: Mycoplasma pneumoniae, Chlamydia pneumoniae, Legionella pneumophila, Haemophilus influenzae, Streptococcus pyogenes (group A), Streptococcus pneumoniae, Candida albicans, Staphylococcus aureus.

#### Interference

The following potential interference substances were evaluated with the COVID-19 Antigen Rapid Test Cassette at the concentrations listed below and were found not to affect test performance.

Substance	Concentration	Substance	Concentration
Mucin	2%	Whole blood	4%
Benzocaine	5 mg/mL	Menthol	10 mg/mL
Saline nasal spray	15%	Phenylephrine	15%
Oxymetazoline	15%	Histamine dihydrochloride	10 mg/mL
Tobramycin	5 µg/mL	Mupirocin	10 mg/mL
Oseltamivir phosphate	10 mg/mL	Zanamivir	5 mg/mL
Arbidol	5 mg/mL	Ribavirin	5 mg/mL
Fluticasone propionate	5%	Dexamethasone	5 mg/mL
Triamcinolone	10 mg/mL		

#### High-dose Hook Effect

The COVID-19 Antigen Rapid Test Cassette was tested up to  $1.0 \times 10^{5.67}$  TCID<sub>50</sub>/mL of inactivated SARS-CoV-2 and no high-dose hook effect was observed.

Hangzhou Clongene Biotech Co., Ltd.  
No.1 Yichuang Road, Yuhang Sub-district, Yuhang District,  
311121 Hangzhou, China

**EC REP** Shanghai International Holding Corp.GmbH (Europe)  
Eiffestrasse 80, D-20537 Hamburg, Germany

#### Index of Symbol

	Do not reuse		For in vitro diagnostic use only
	Store between 4-30°C		Consult instructions for use
	Lot number		Contains sufficient for <n> tests
	Use by		Keep away from sunlight
	Keep dry		Do not use if package is damaged
	Manufacturer		Authorized representative in the European Community

Version No.: 3.0  
Effective Date: October 26, 2020